

500

600

700

800


900

1000

1100

1200

(2)

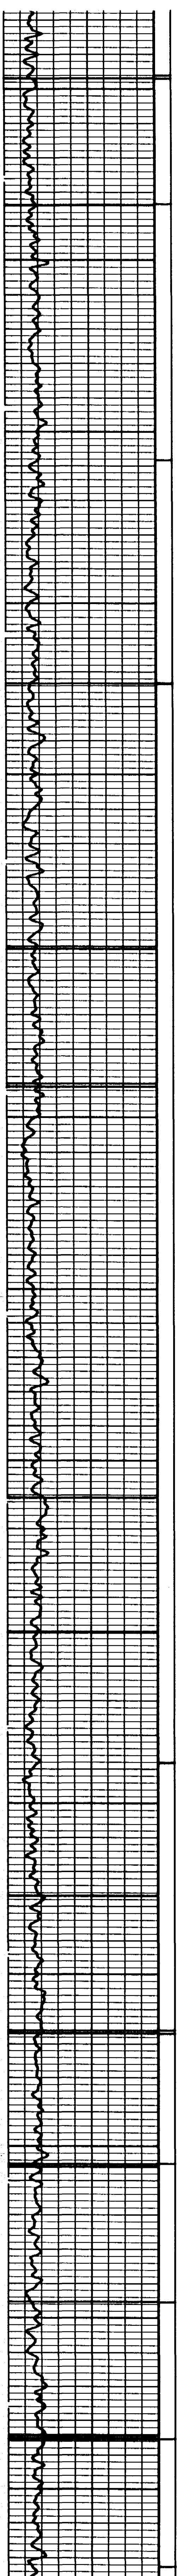

1300

1400


1500

1600



1700

1800

1900

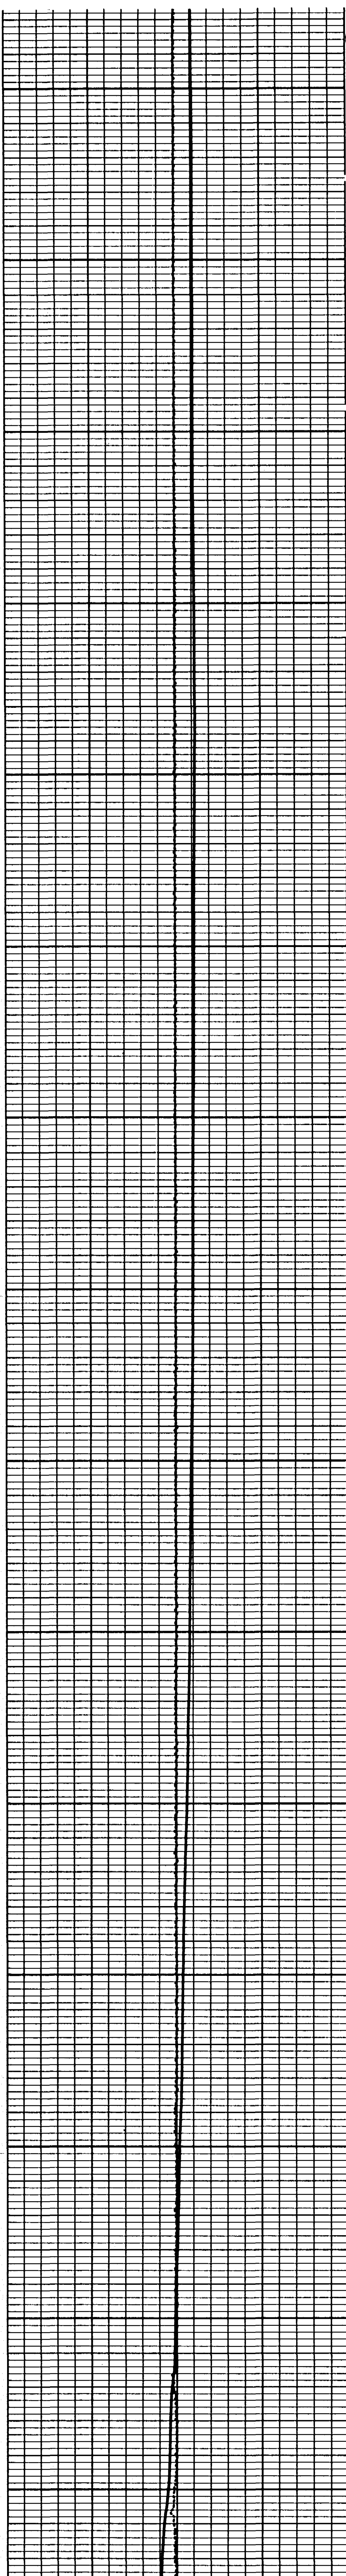

(17)

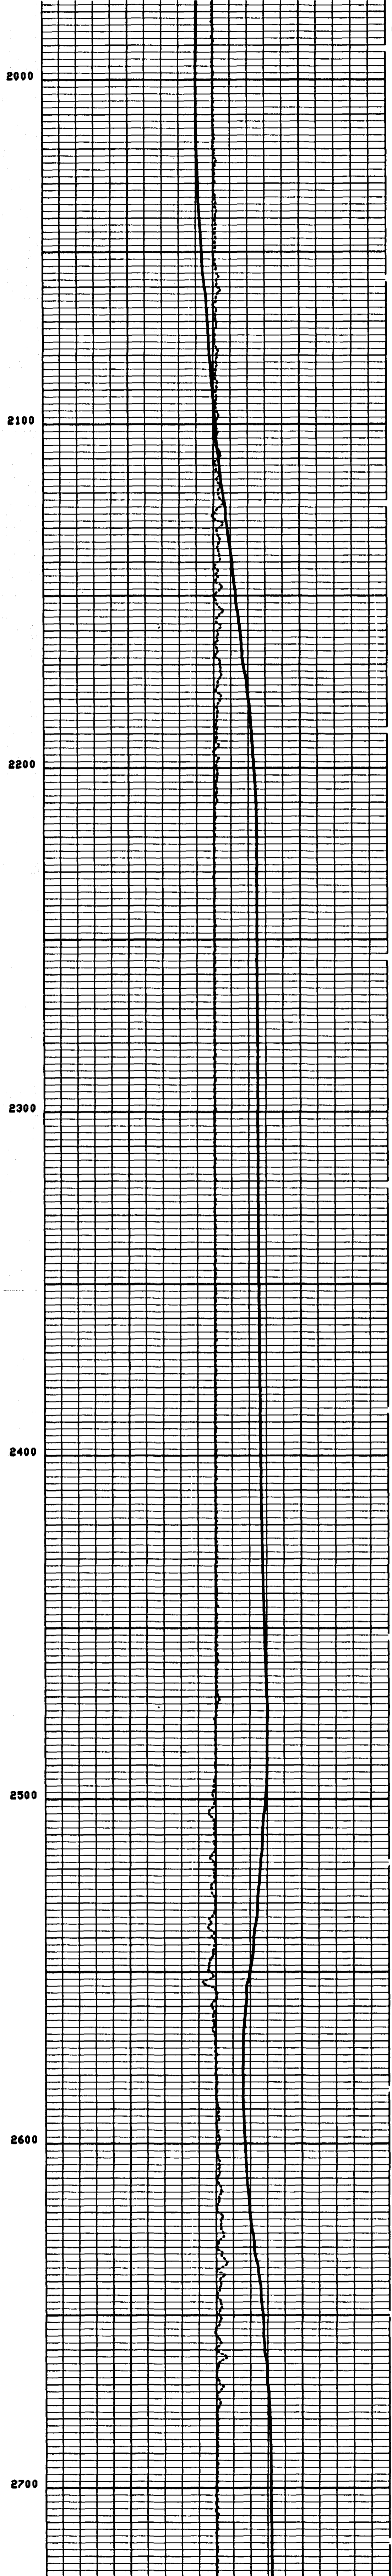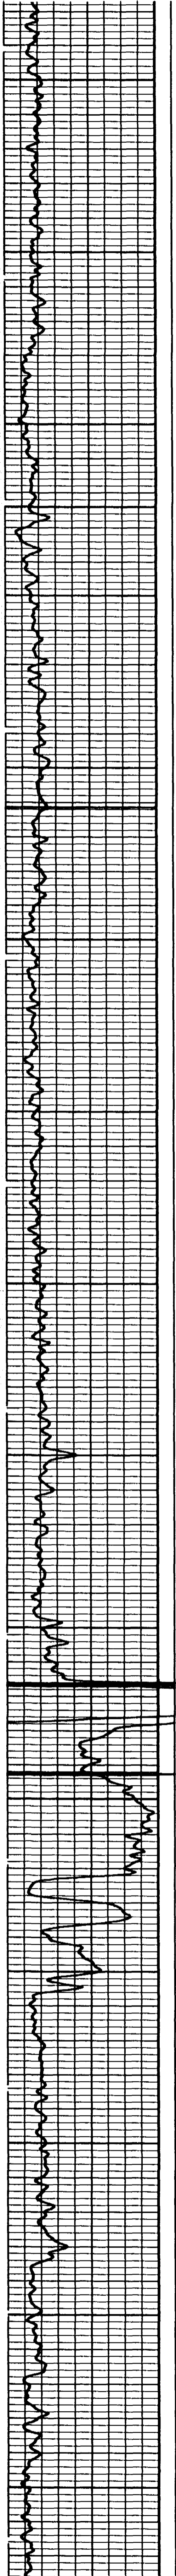

2000

2100

2200


2300

2400

2500

2600

2700

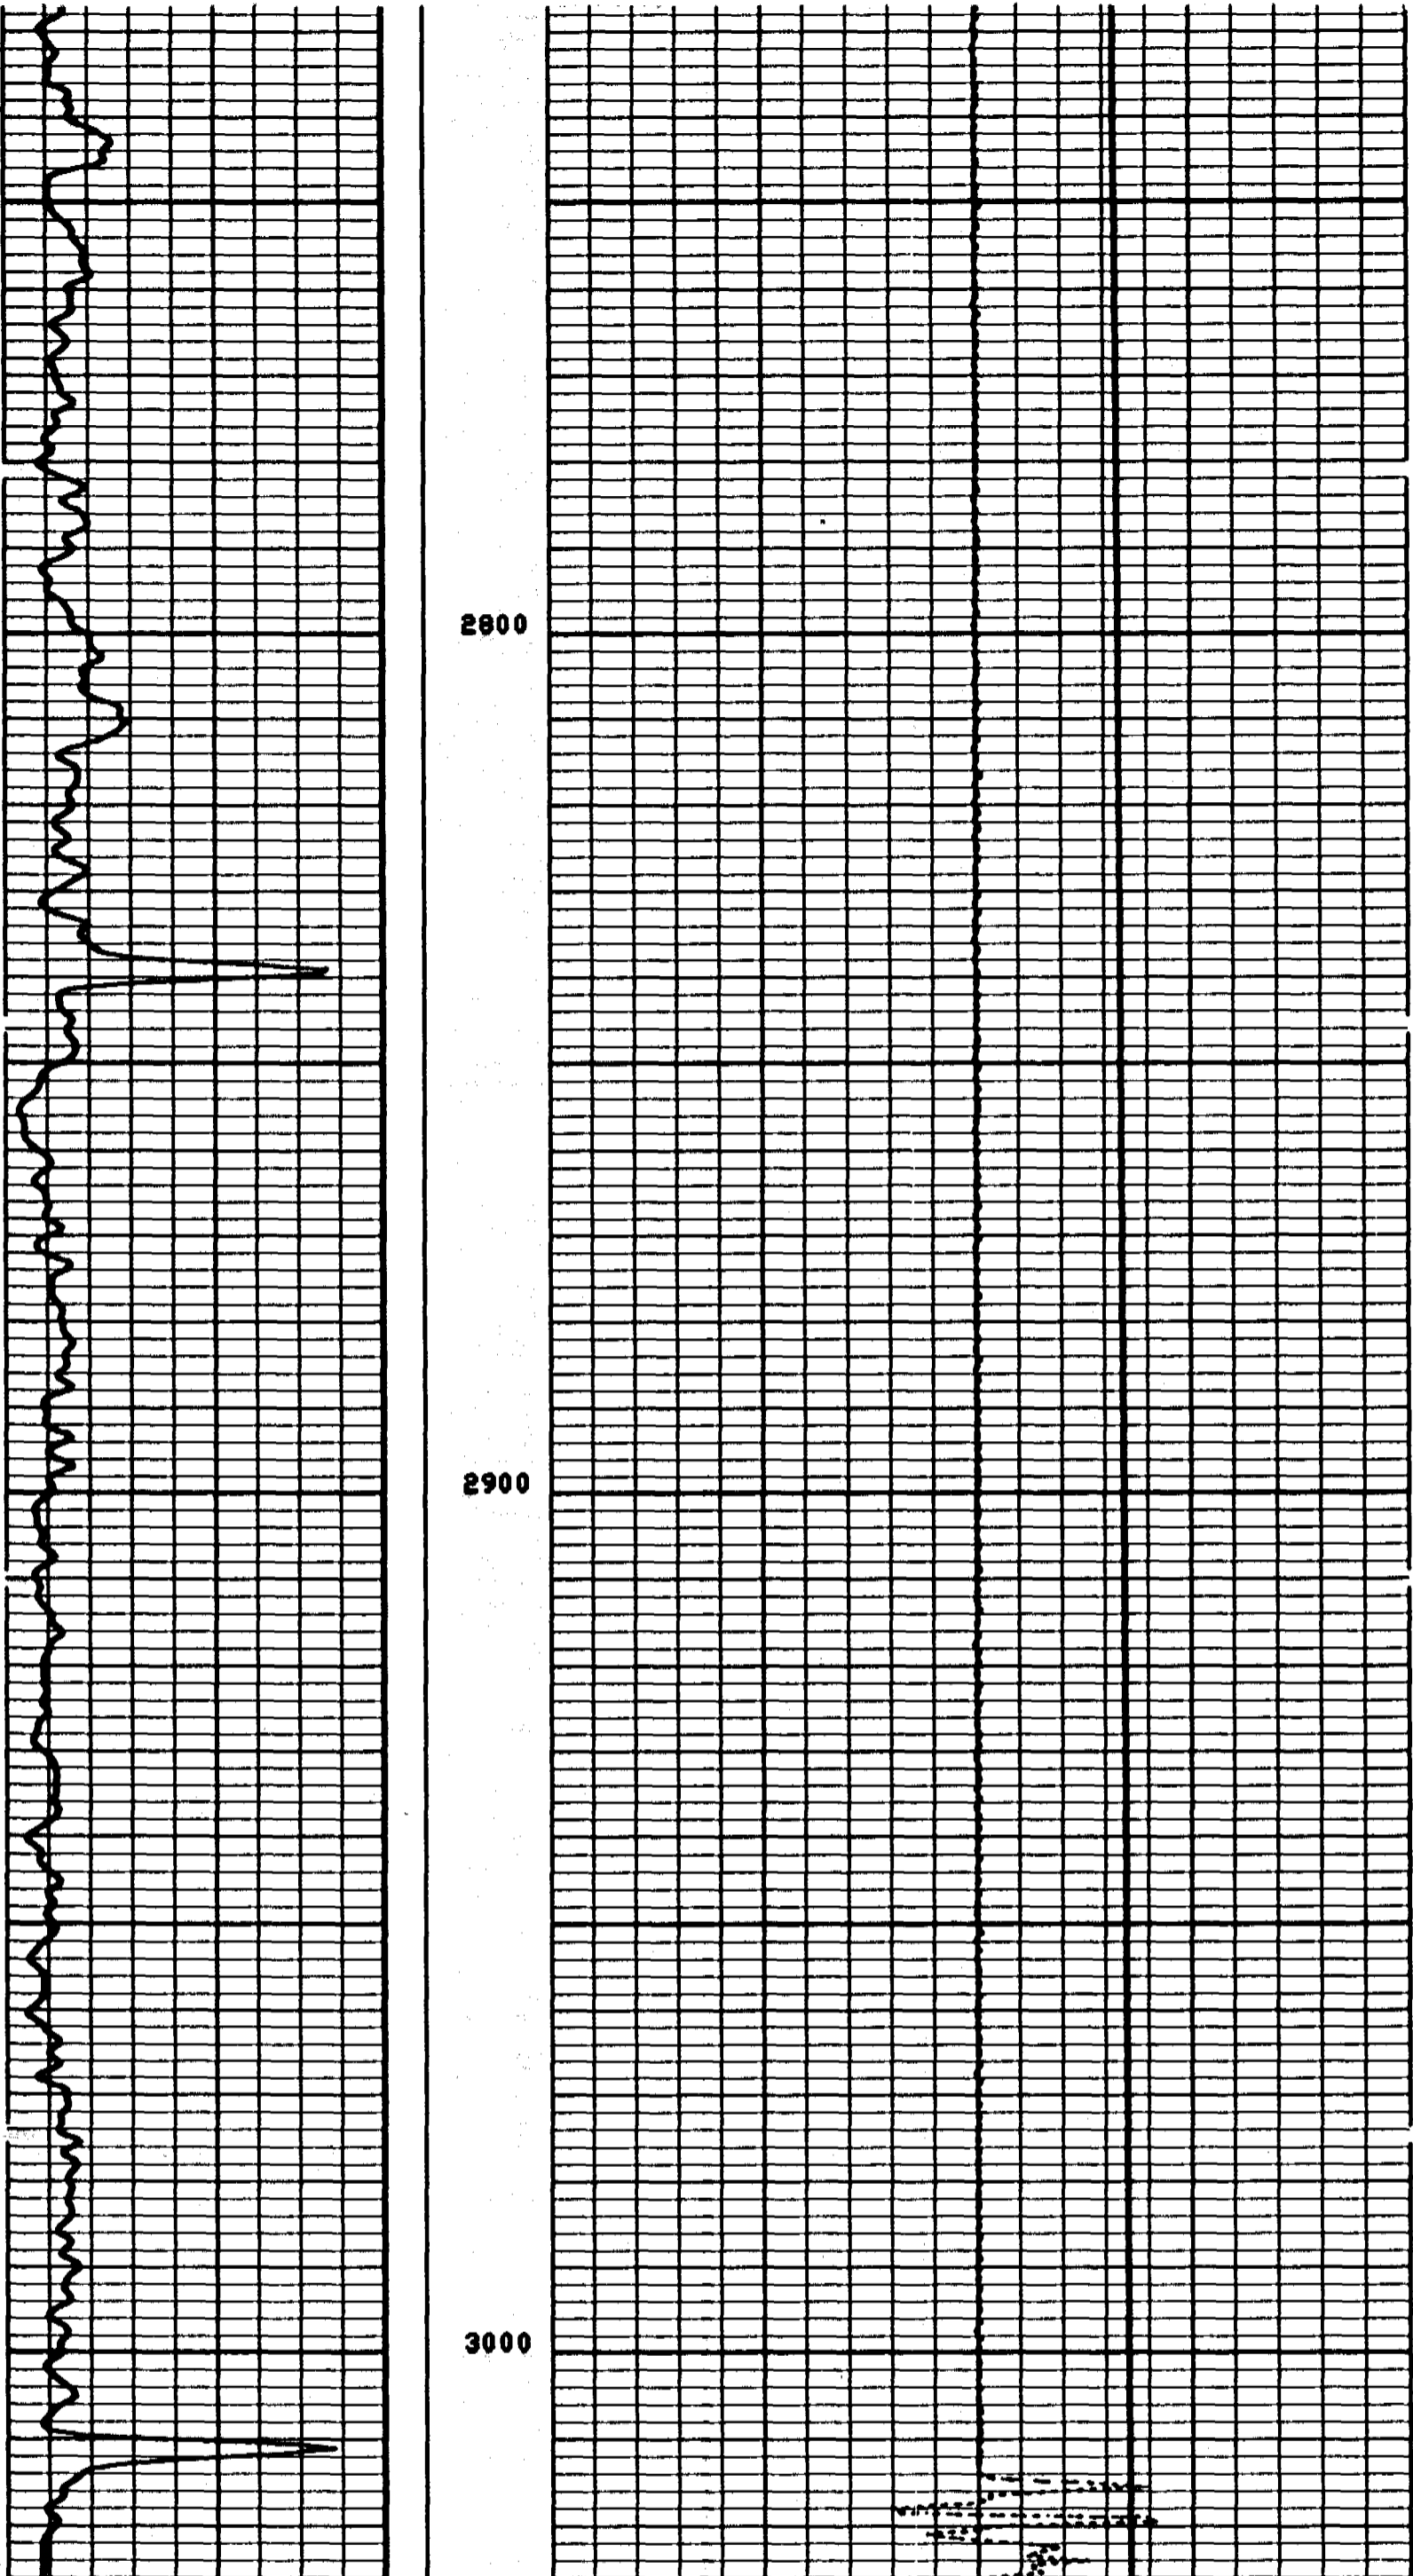

CP 32.2 FILE 1 04-MAY-1991 00:01
 INPUT FILE(S) DATA ACQUIRED
 2 04-MAY-1991 14:08

GR (GAPI)	0.0	100.00	TEMP(DF/F)	-1.000	1.0000
CCL	-13.50	1.5000	TEMP(DEGF)	20.000	90.000

BEFORE SURVEY CALIBRATION SUMMARY

PERFORMED: 04-MAY-1991 13:12
 PROGRAM FILE: PL (VERSION 32.2 00/00/00 88/11/16)

	MEASURED		CALIBRATED		
MP	ZERO	PLUS	ZERO	PLUS	UNITS
	0.0	0.0	0.0	0.0	PSIG

MTSC ELECTRONICS CALIBRATION SUMMARY

	MEASURED		CALIBRATED		
TEMP	ZERO	PLUS	ZERO	PLUS	UNITS
	57.8	173.8	0.0	200.0	DEGF

CP 32.2 FILE 0 04-MAY-1991 13:12